


# COUPP/PICO Operations Summary

Ended both COUPP-60 and PICO-2L in the last two weeks

- Both runs ended without incident
- Target fluids safely drained and detectors are now idle and un-pressurized
- Collected large calibration data sample in COUPP-60 over last several weeks, PICO-2L ran in dark matter search mode until the end
- Currently making a temperature measurement in PICO-2L to confirm our understanding of the thermodynamic conditions
- Plan for June is to begin a careful sampling of the remaining fluids, looking primarily for particulate contamination
- To be followed by a refill of PICO-2L with a new buffer fluid (LAB liquid scintillator)
- COUPP60 plan will be determined once sampling results are in hand

# COUPP-60 2013-2014 Run

## Final Exposure Vs. Time

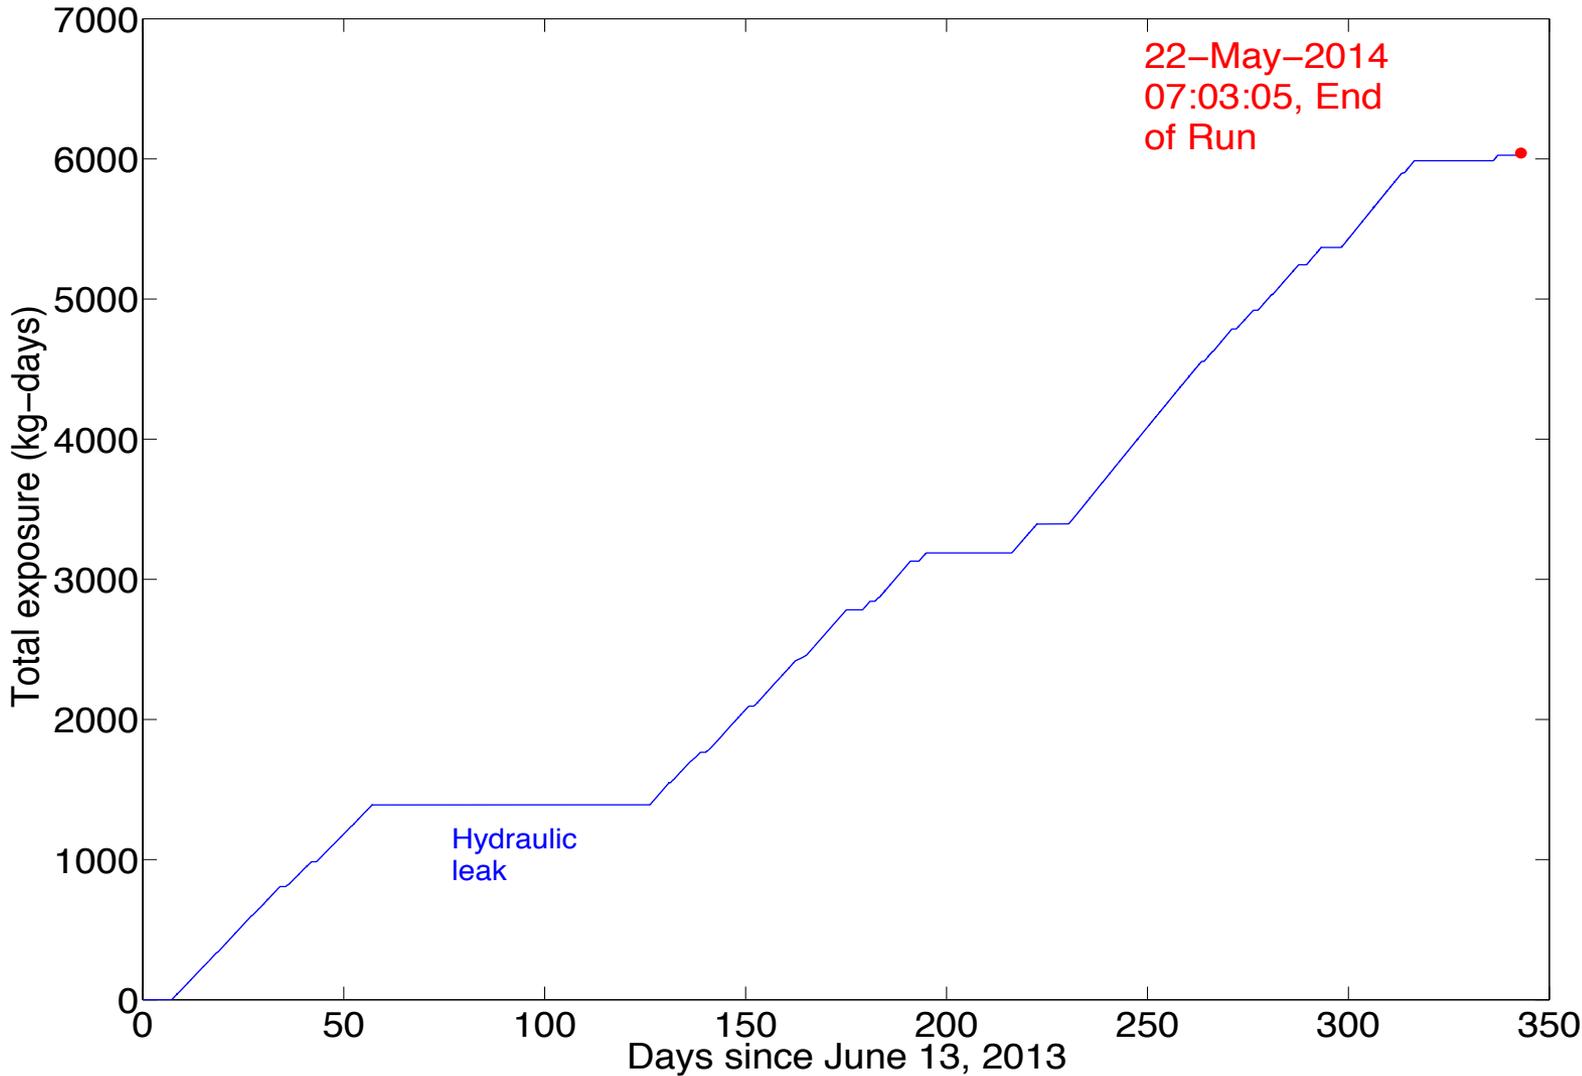

# PICO-2L 2013-2014 Run Final Exposure Vs. Time

